

This Page Is Inserted by IFW Operations  
and is not a part of the Official Record

## **BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning documents *will not* correct images,  
please do not report the images to the  
Image Problem Mailbox.**

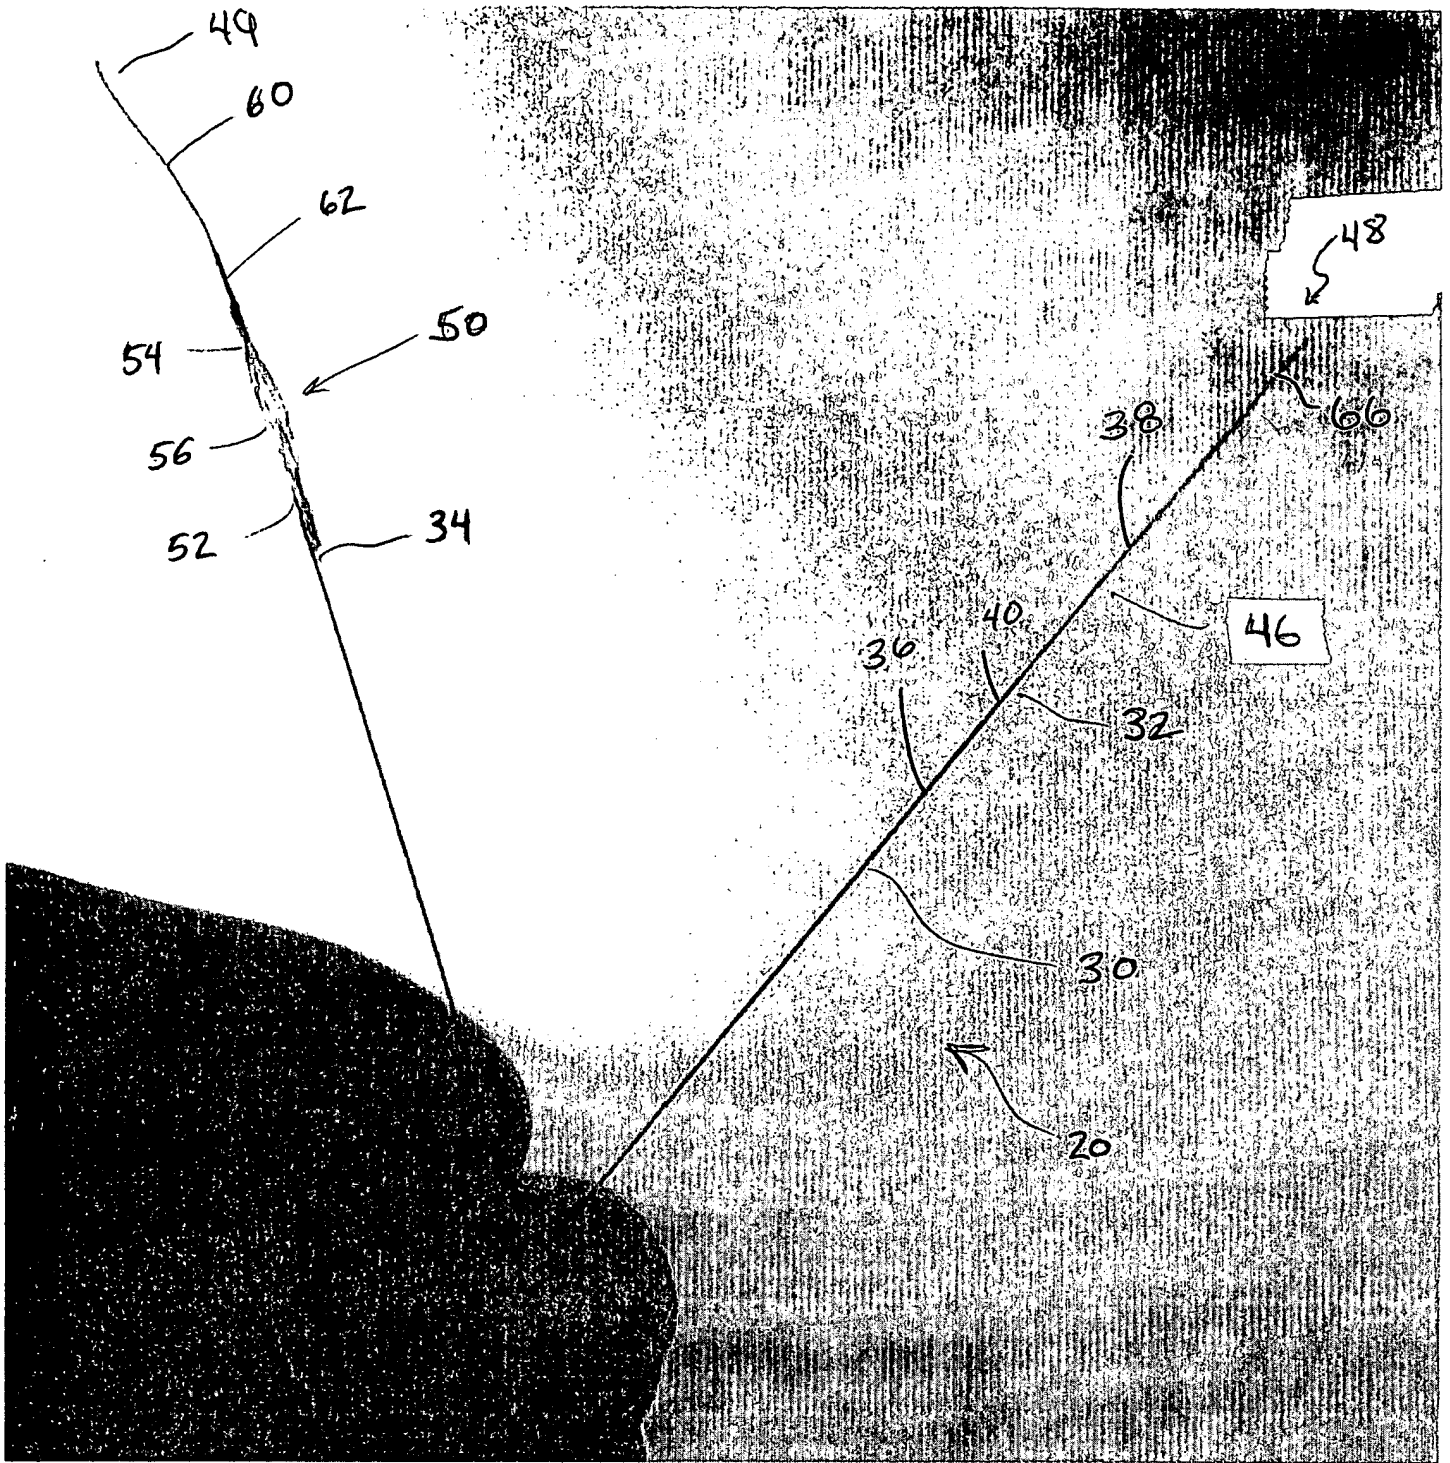


FIGURE 1

**FIGURE 2**

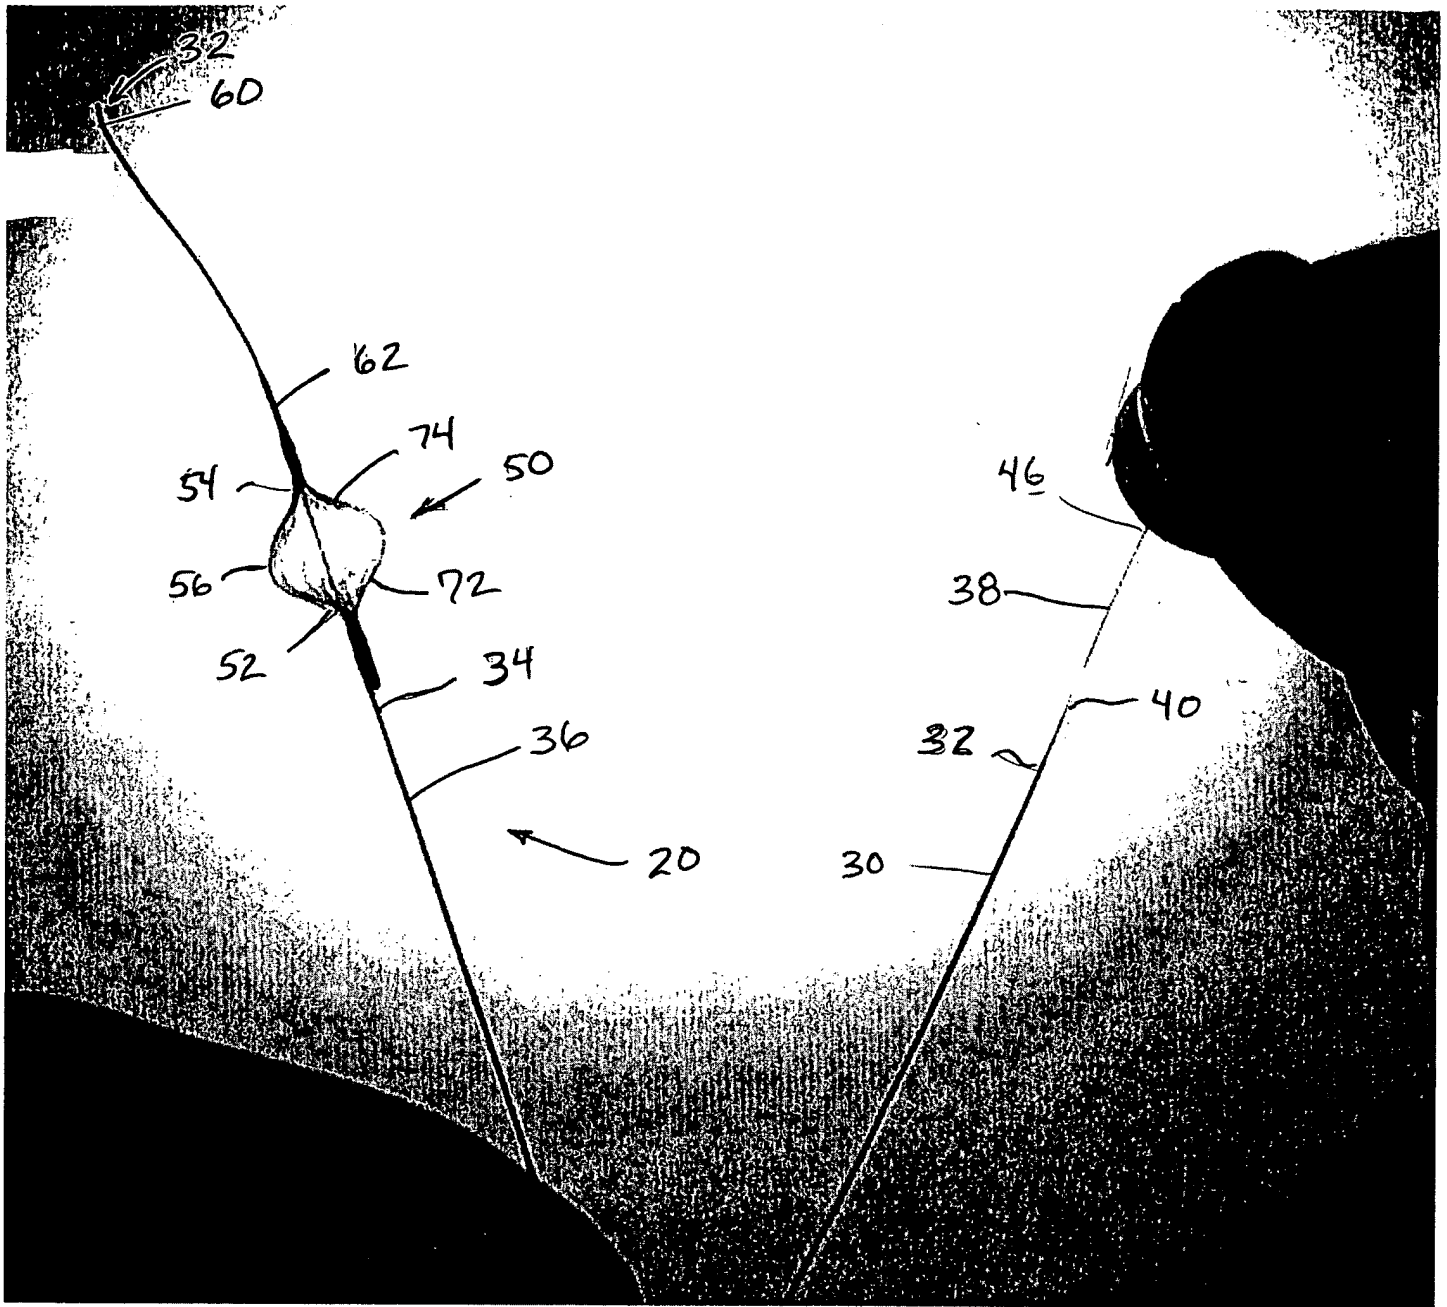
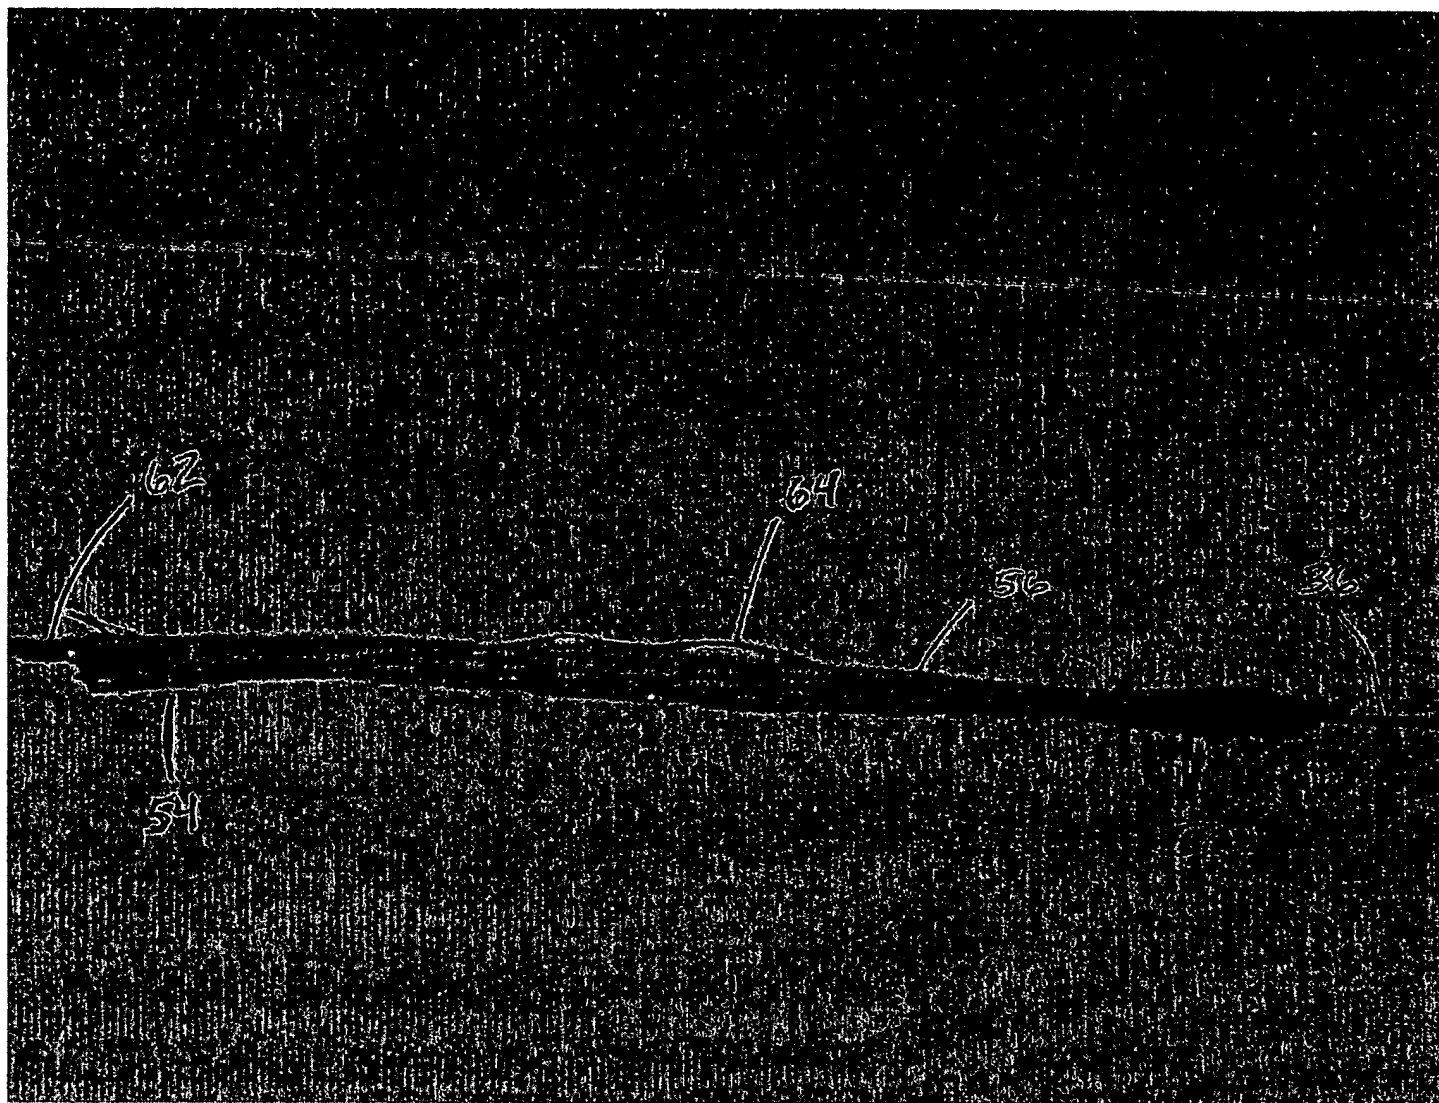


Figure 3



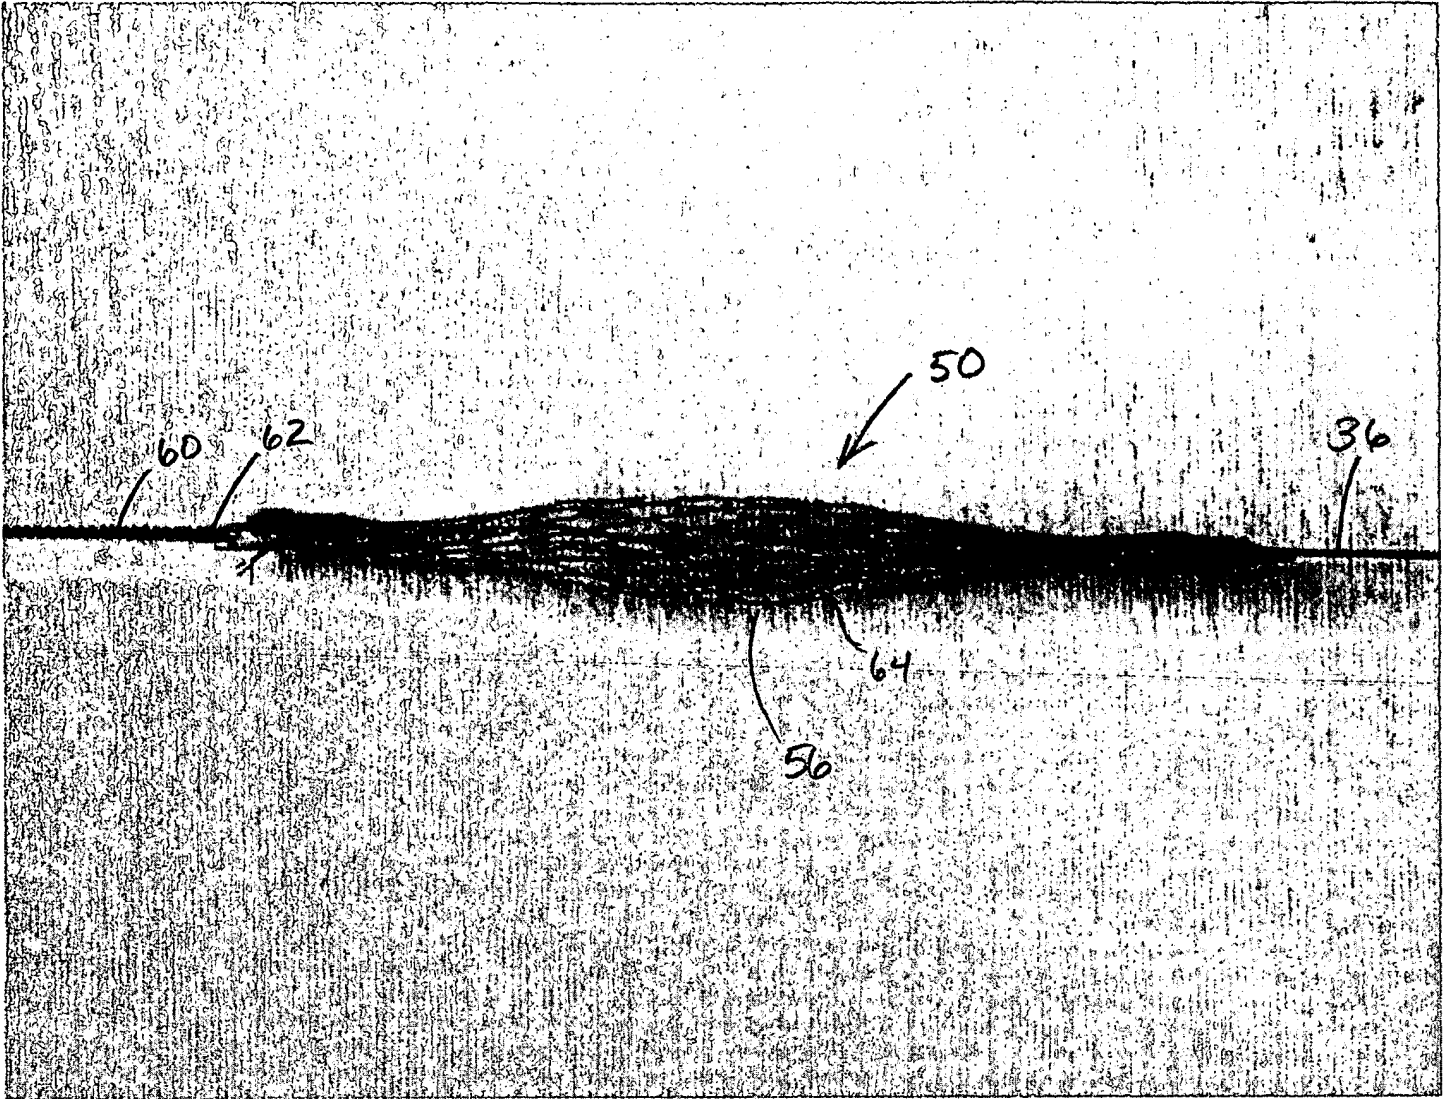


Figure 4

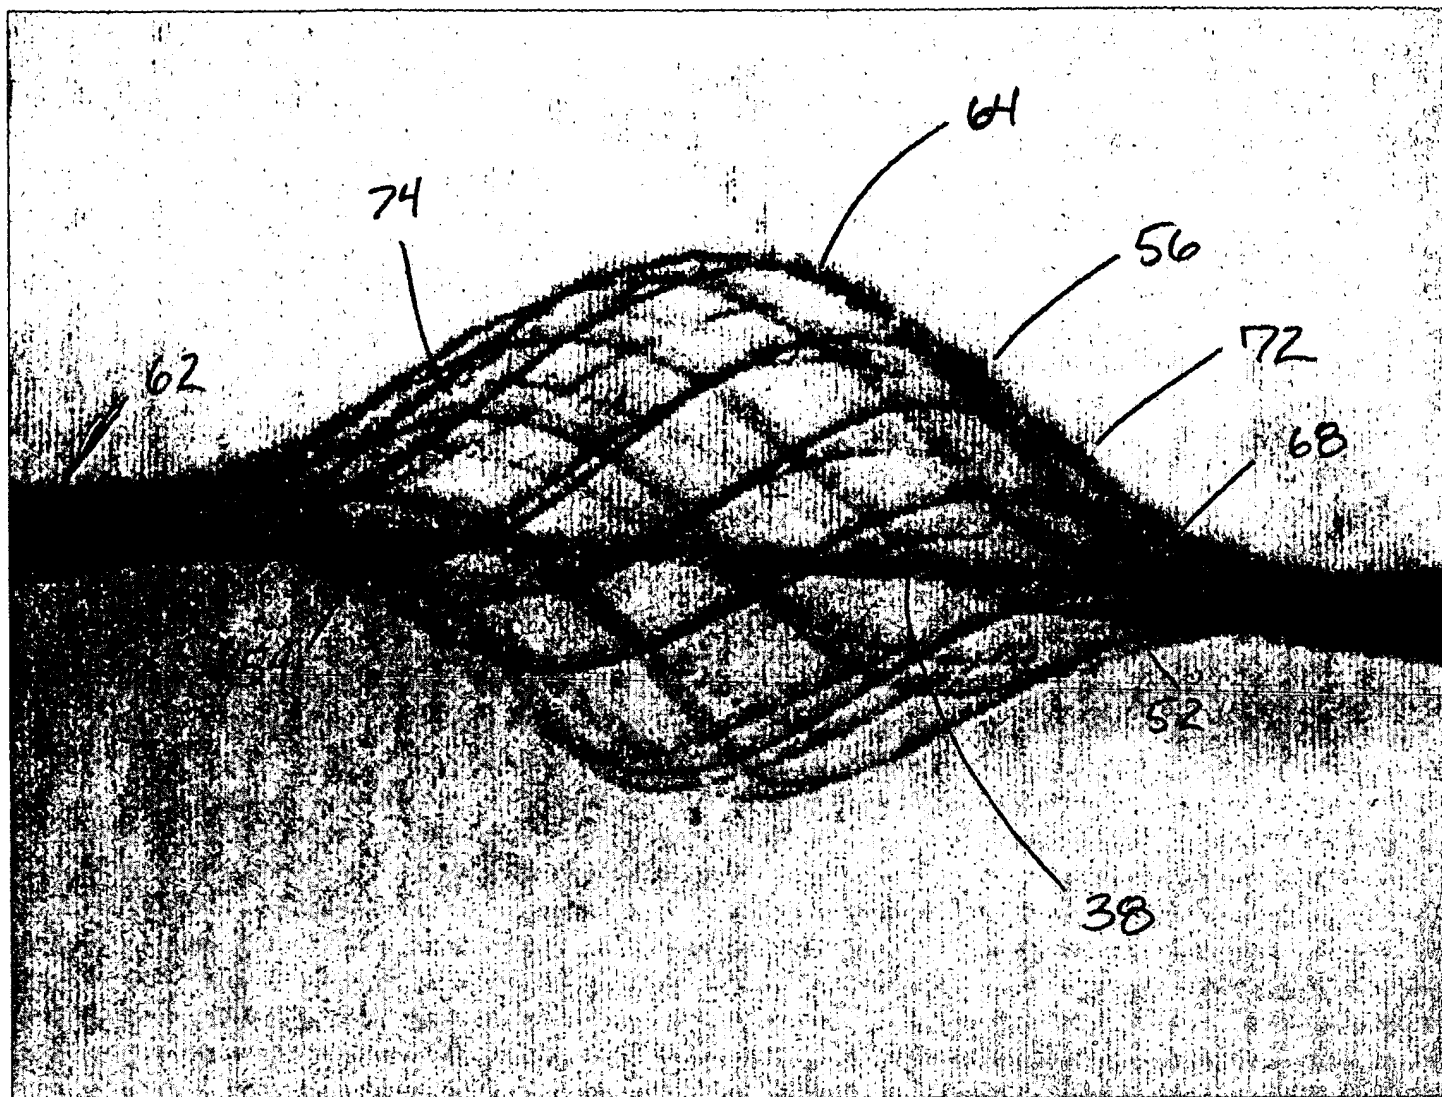


Figure 5

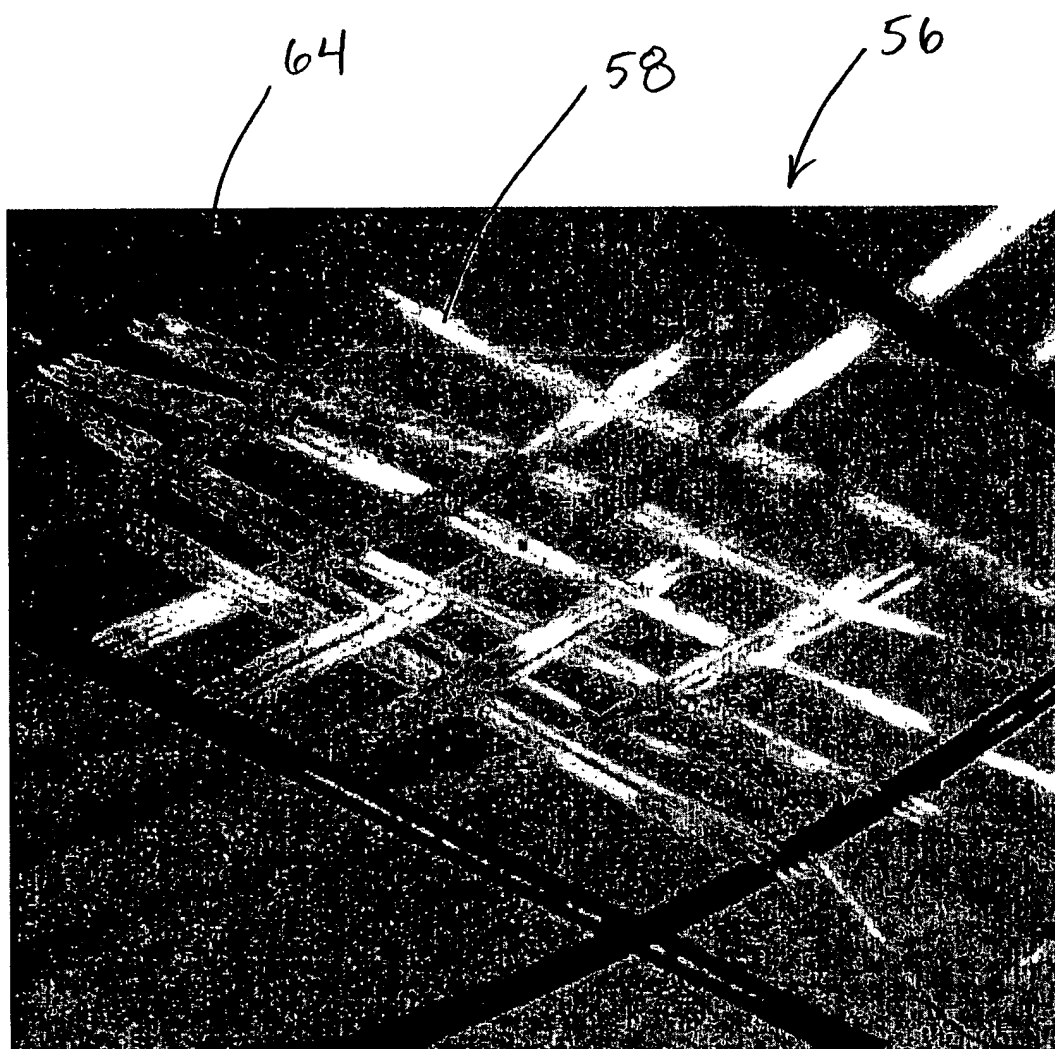


Figure 6

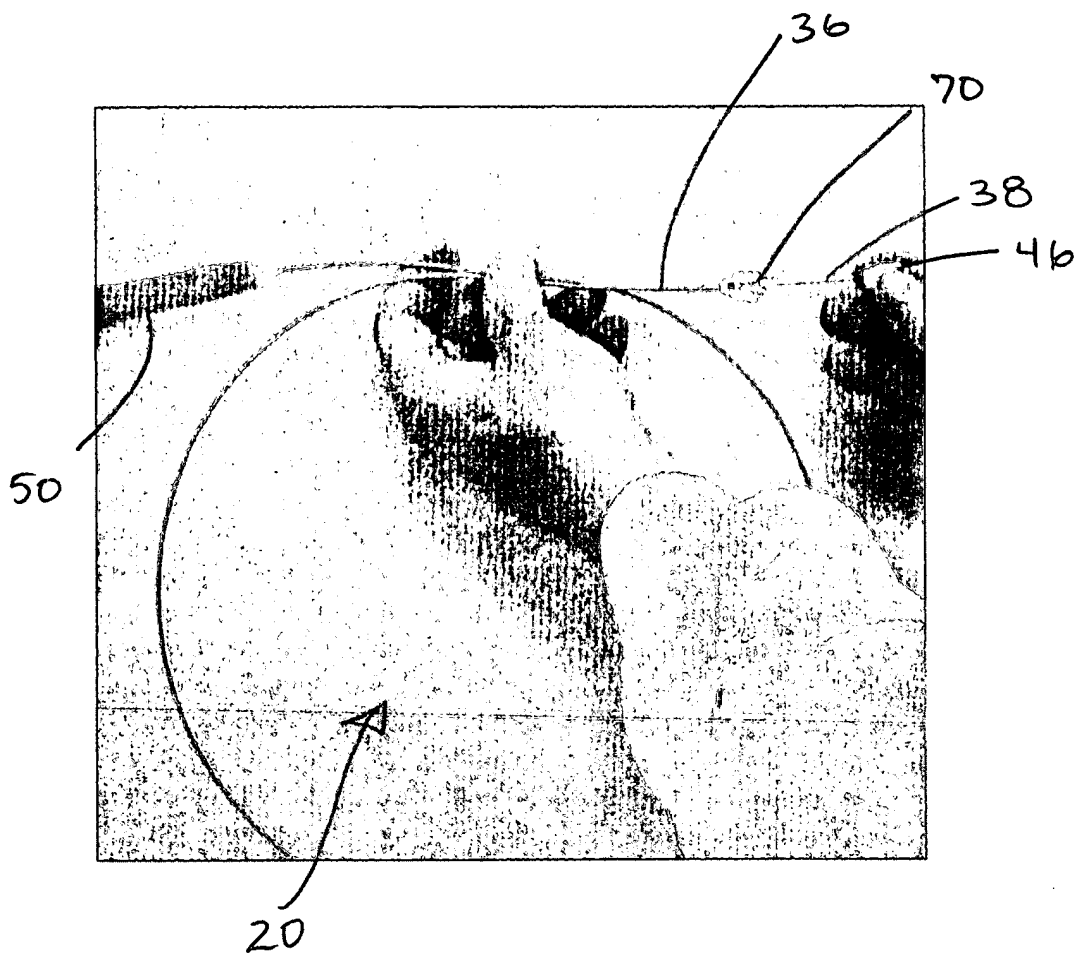


Figure 7



50

185 CM

7 CM

10 MM

3.5 CM

4 CORE

$\phi 0.095$

$\phi 0.150$  (M AX)

1 BRAIDED POLYMER TUBE

3 BRAIDED NITINOL FILTER

49 BOND

5 DISTAL CORE SPRING

2 DISTAL GROUND CORE



A


B

$\phi 0.141$

POSSIS		00 NOT SCALE DRAWING		ALL DIMENSIONS SHOWN IN INCHES UNLESS OTHERWISE SPECIFIED TOLERANCES ARE: FRACTIONS DECIMALS FRACTIONS DECIMALS FRACTIONS DECIMALS	
Bringing Medical Professionals in Life		SEE BOM		NO TOLERANCES RELIEVED UNLESS OTHERWISE SPECIFIED	
DATE: 8/22/2003		7		10. TOLERANCES RELIEVED UNLESS OTHERWISE SPECIFIED	
BY: MHH		10. TOLERANCES RELIEVED UNLESS OTHERWISE SPECIFIED		11. TOLERANCES RELIEVED UNLESS OTHERWISE SPECIFIED	
CONCEPT		01		12. TOLERANCES RELIEVED UNLESS OTHERWISE SPECIFIED	
SIZE		1 1/2		13. TOLERANCES RELIEVED UNLESS OTHERWISE SPECIFIED	
1 1/2		2		14. TOLERANCES RELIEVED UNLESS OTHERWISE SPECIFIED	

168

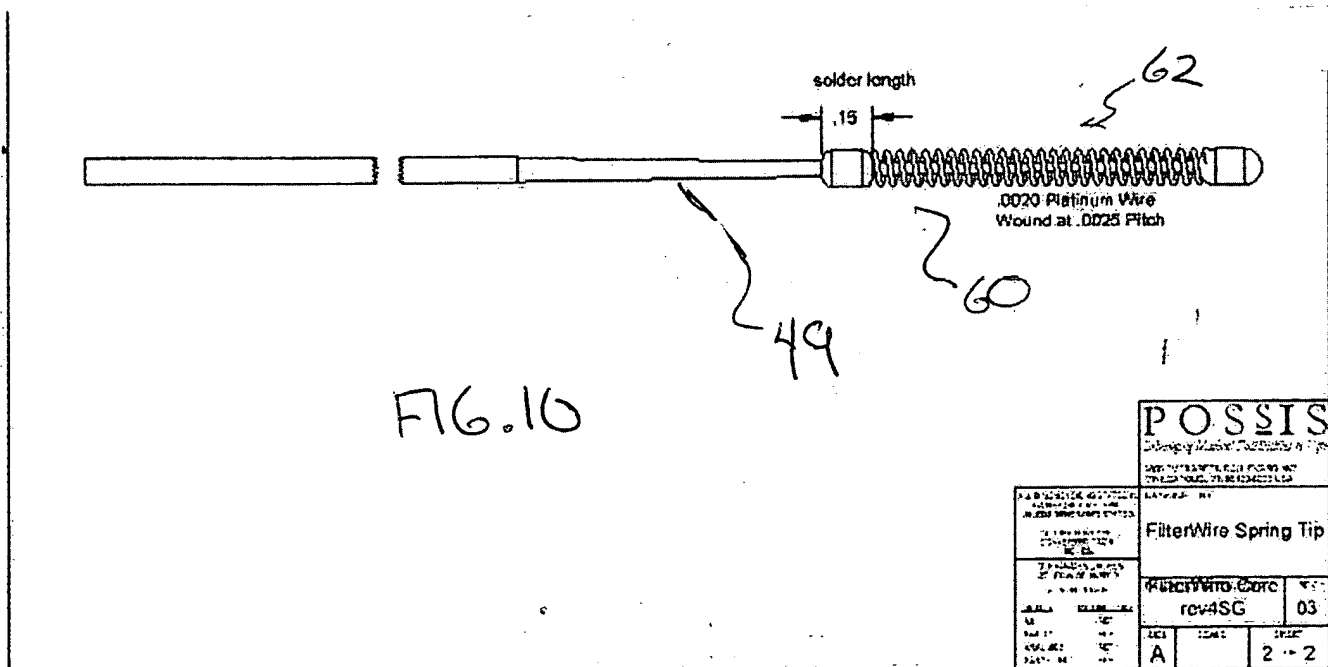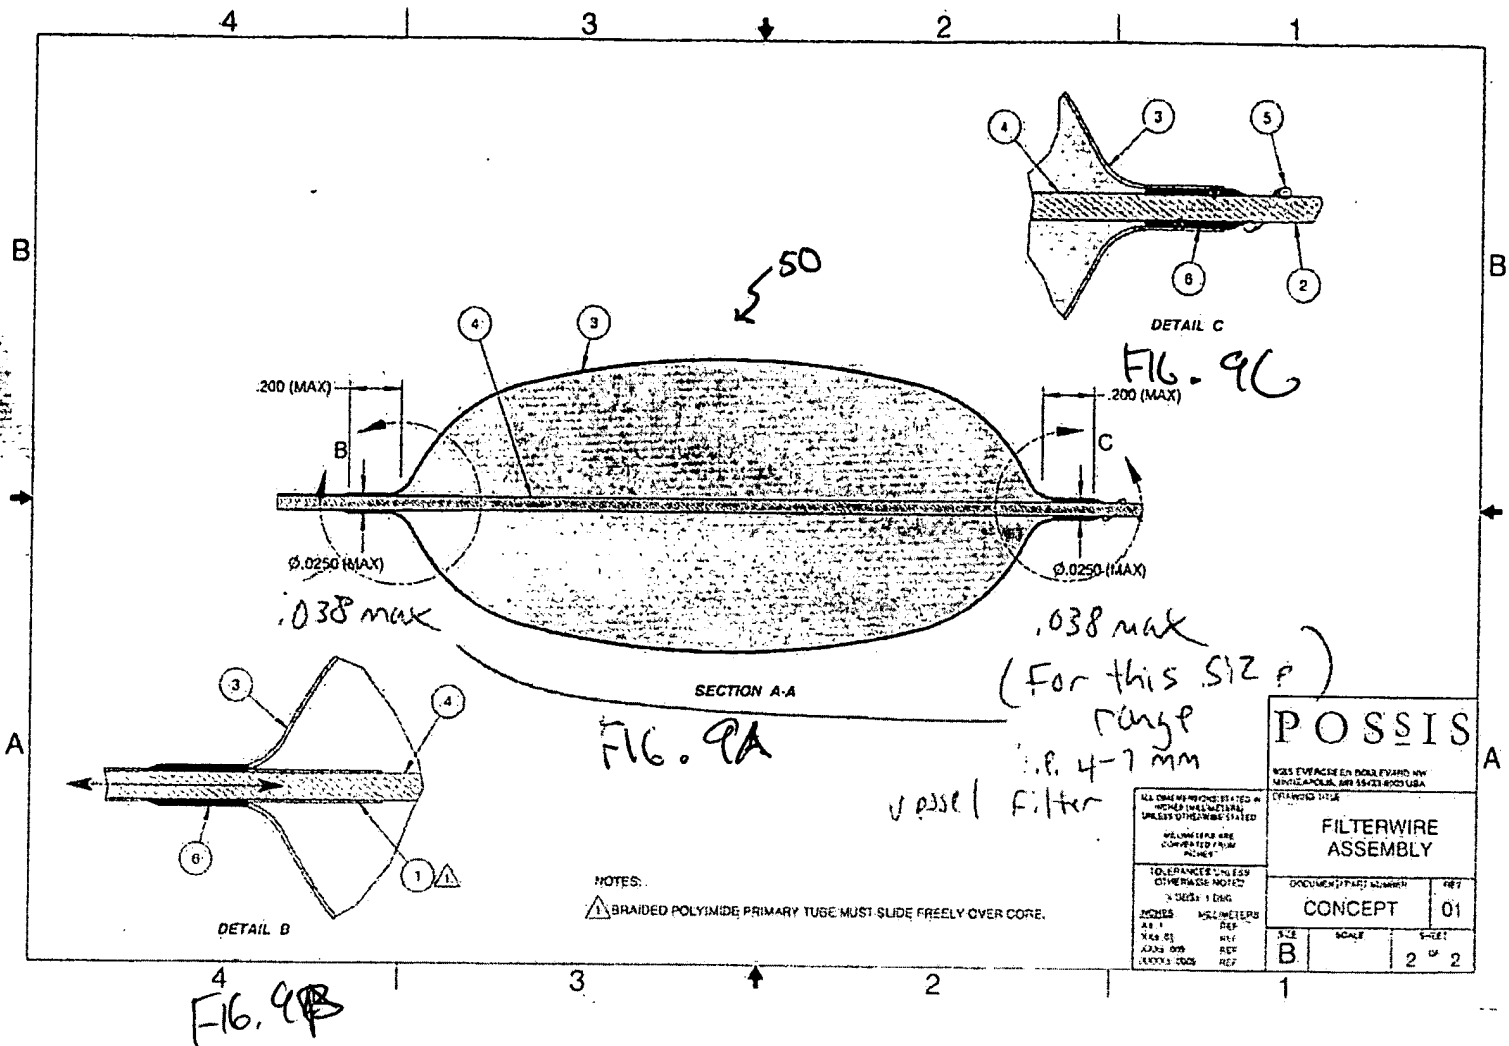

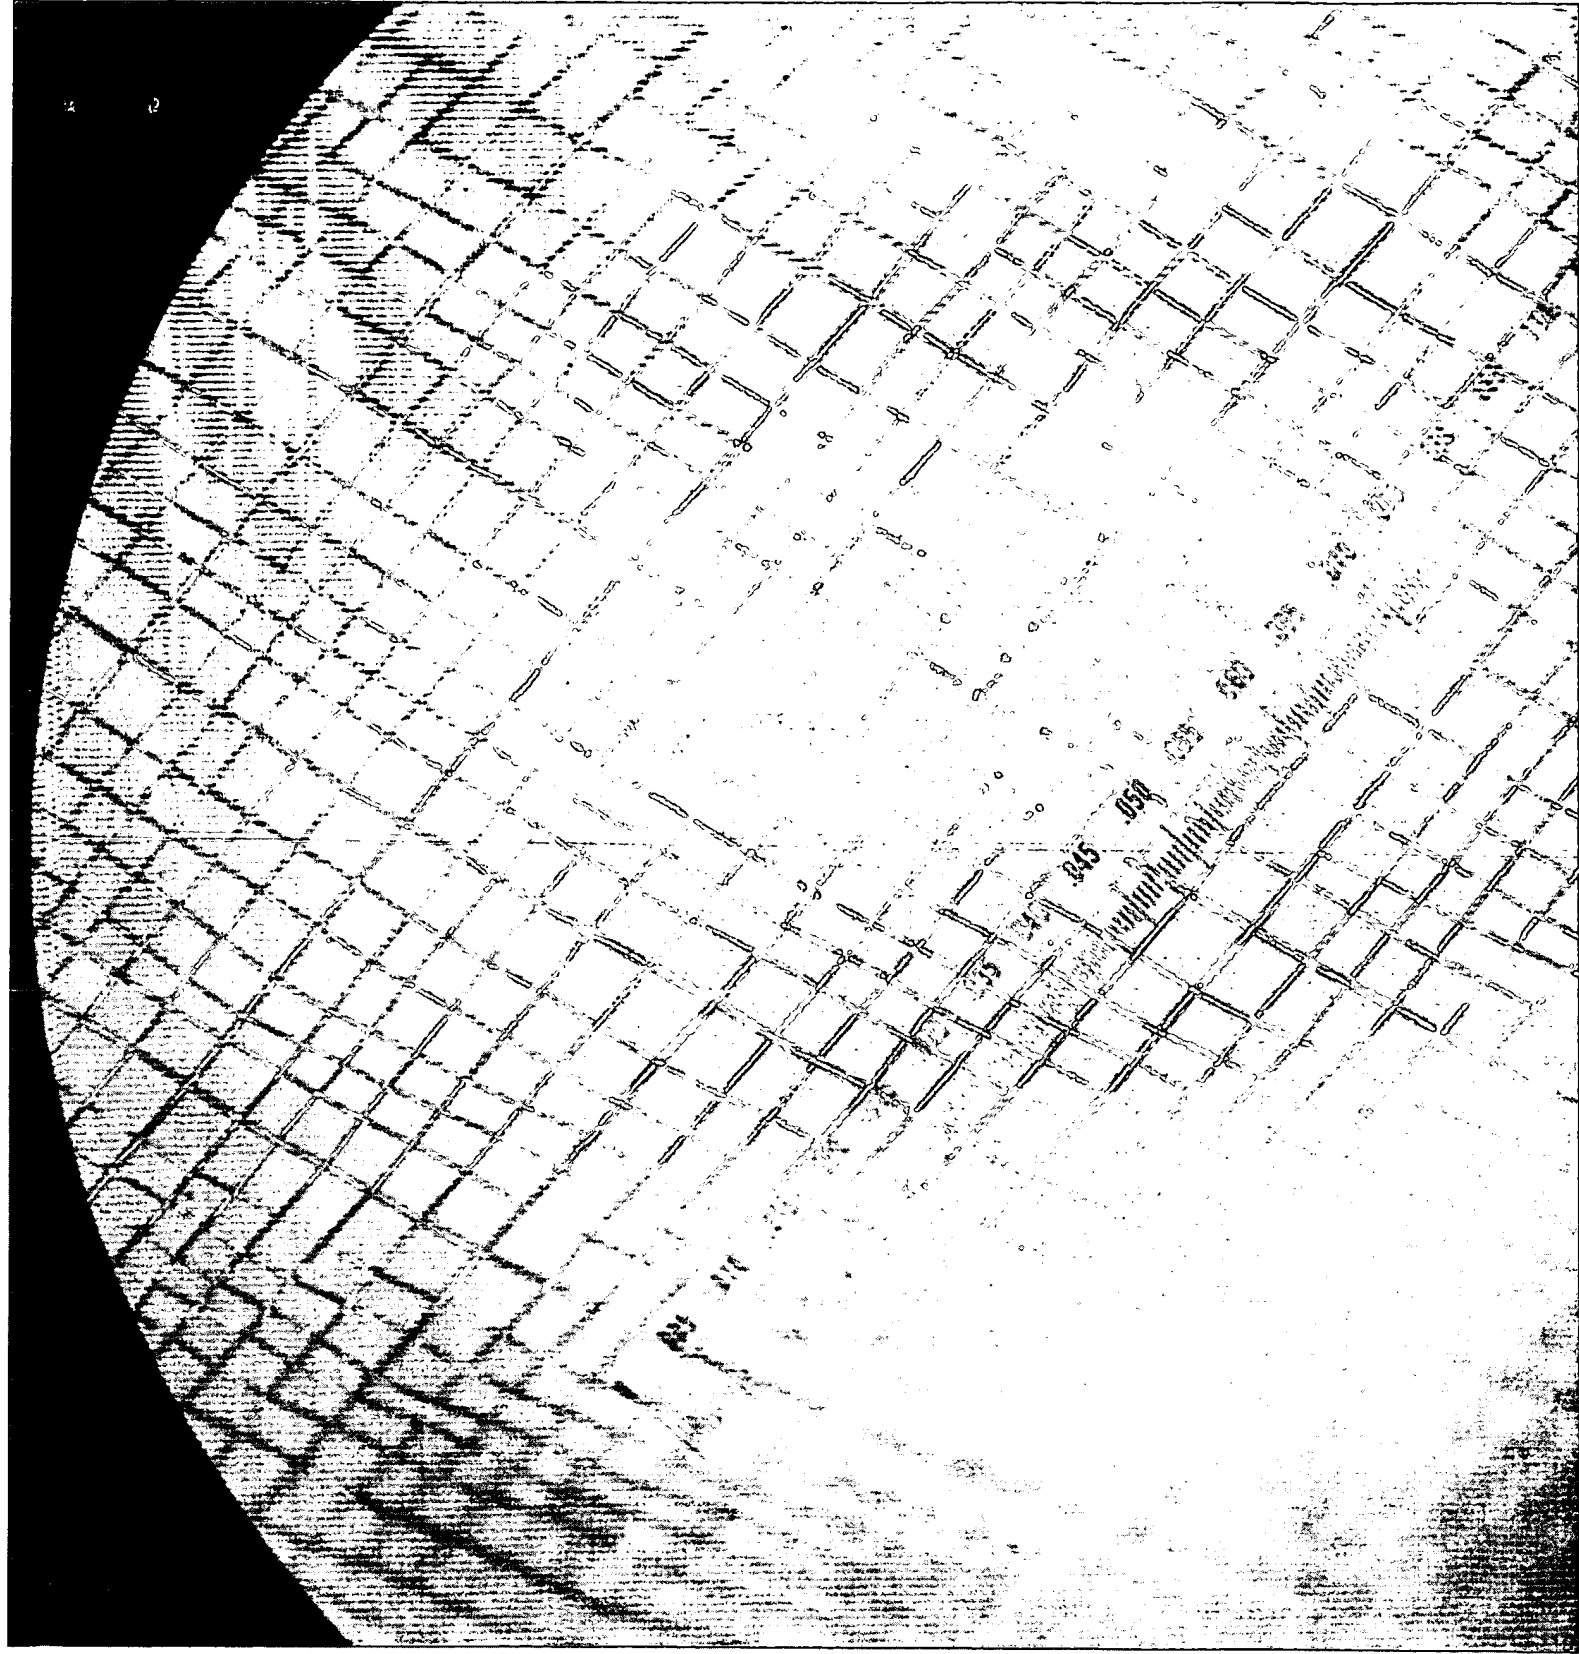

Fl6.11

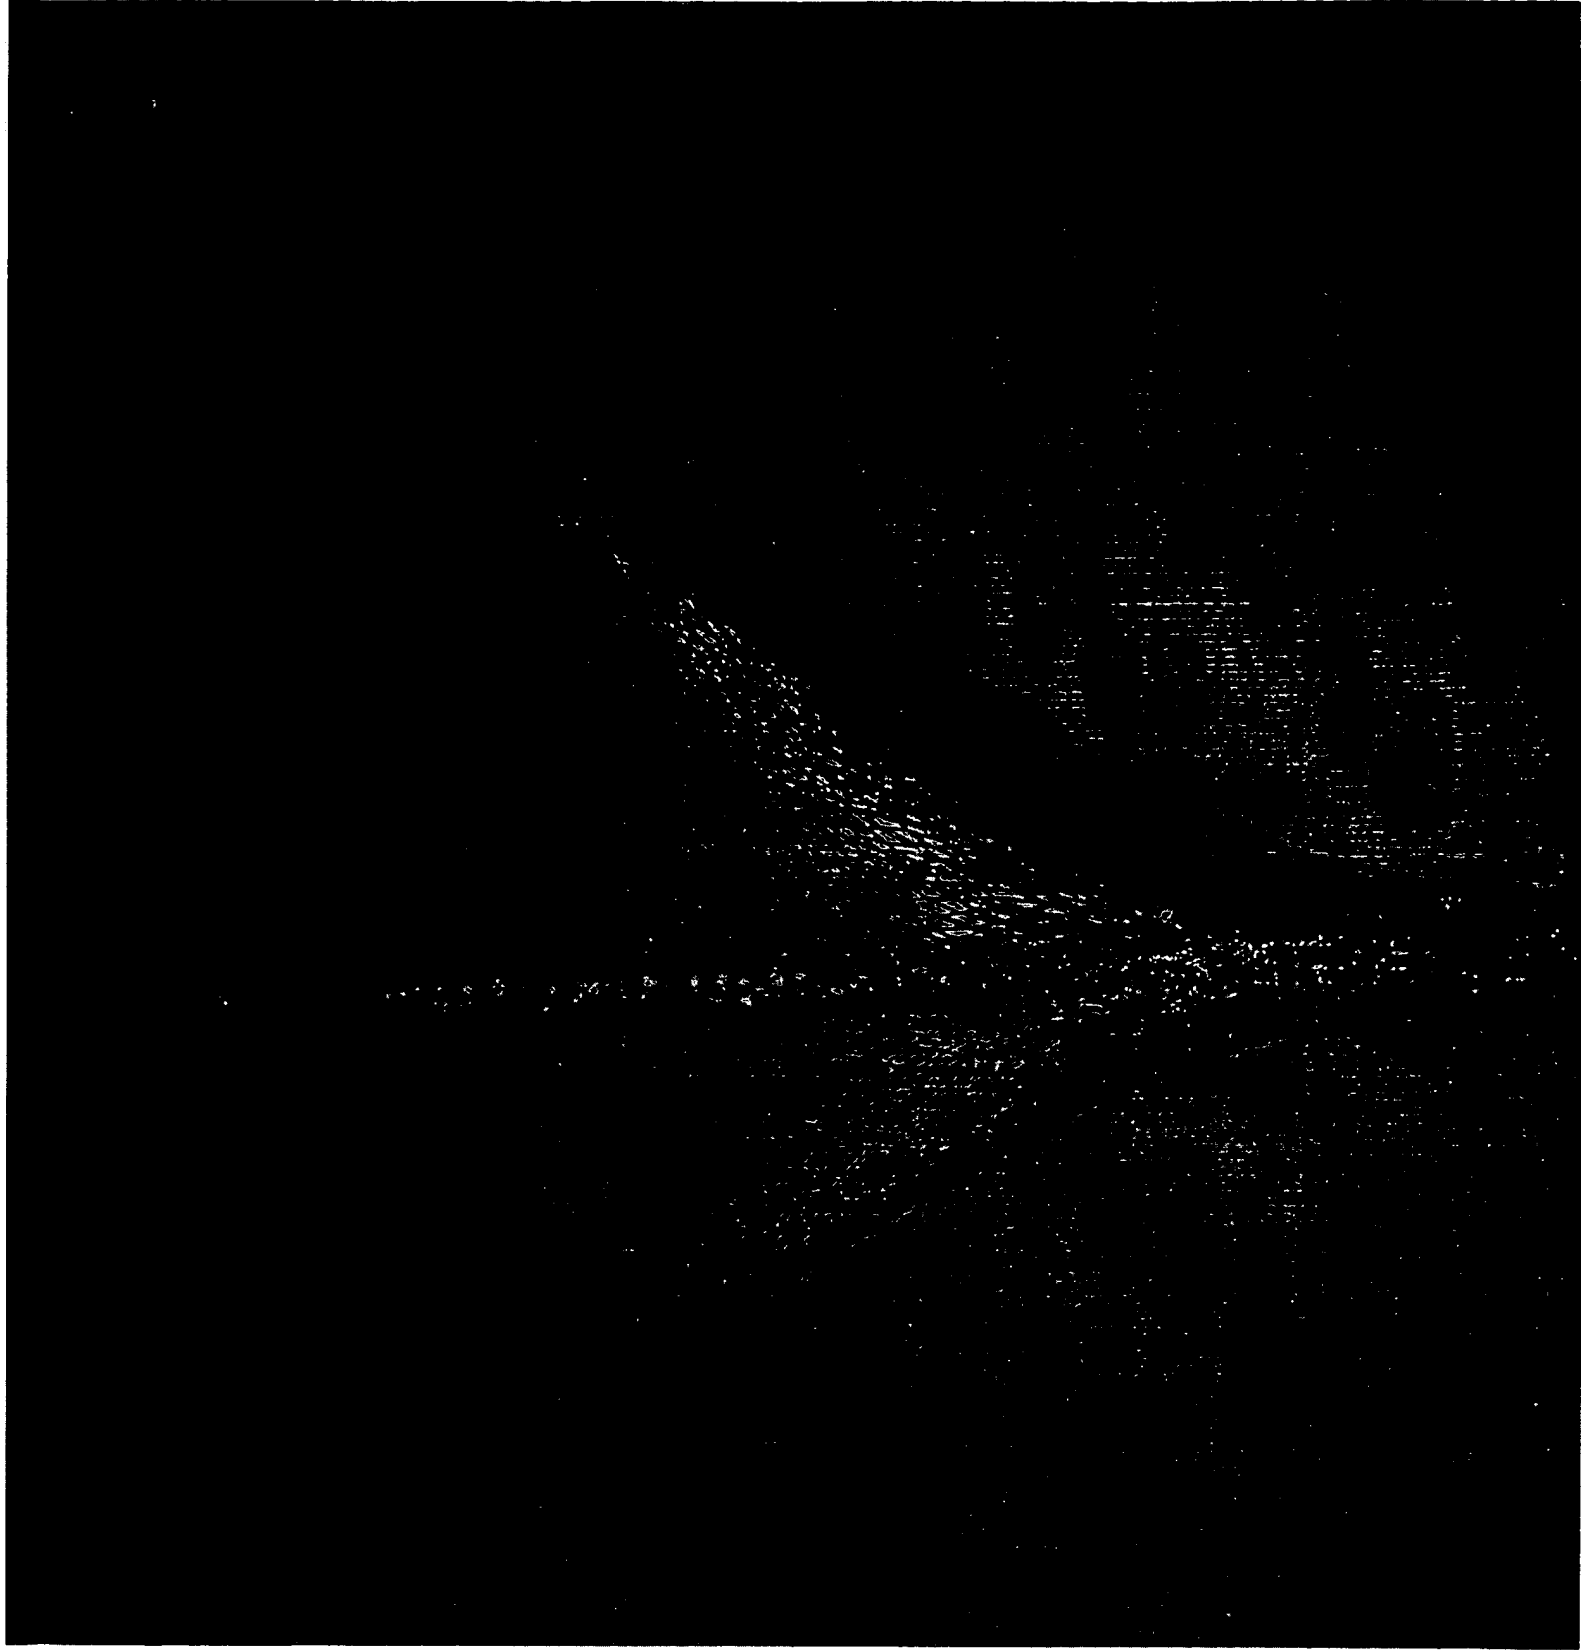


Fig. 12

FIG. 13

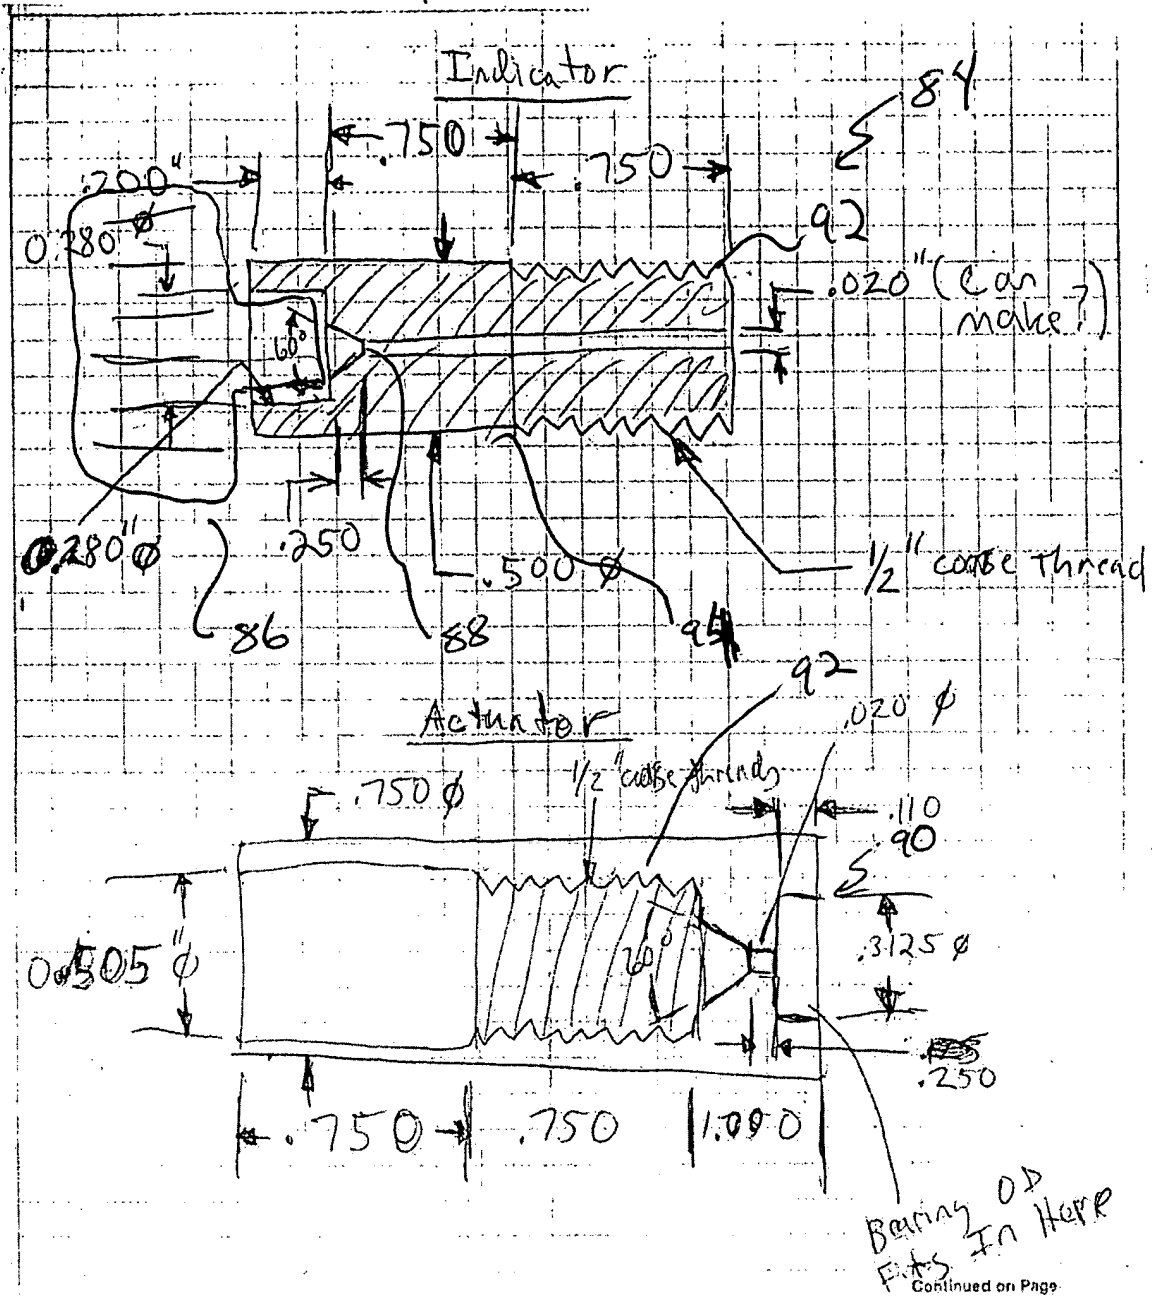


FIG. 14

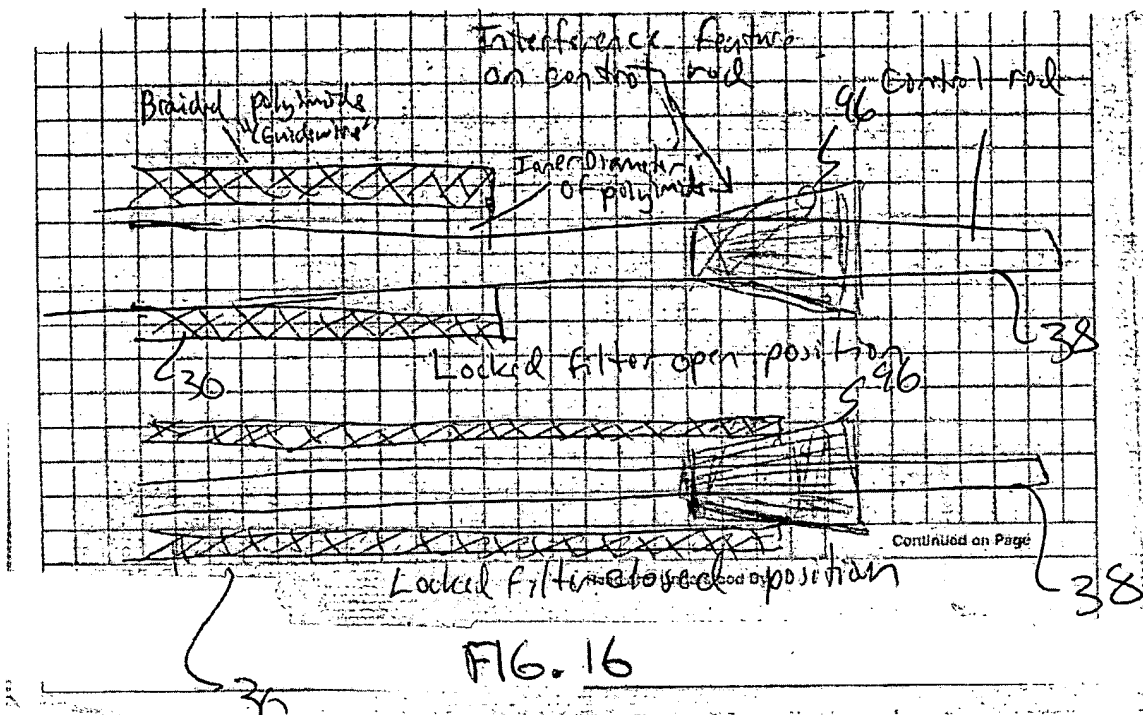


FIG. 16